

Fig. 1.

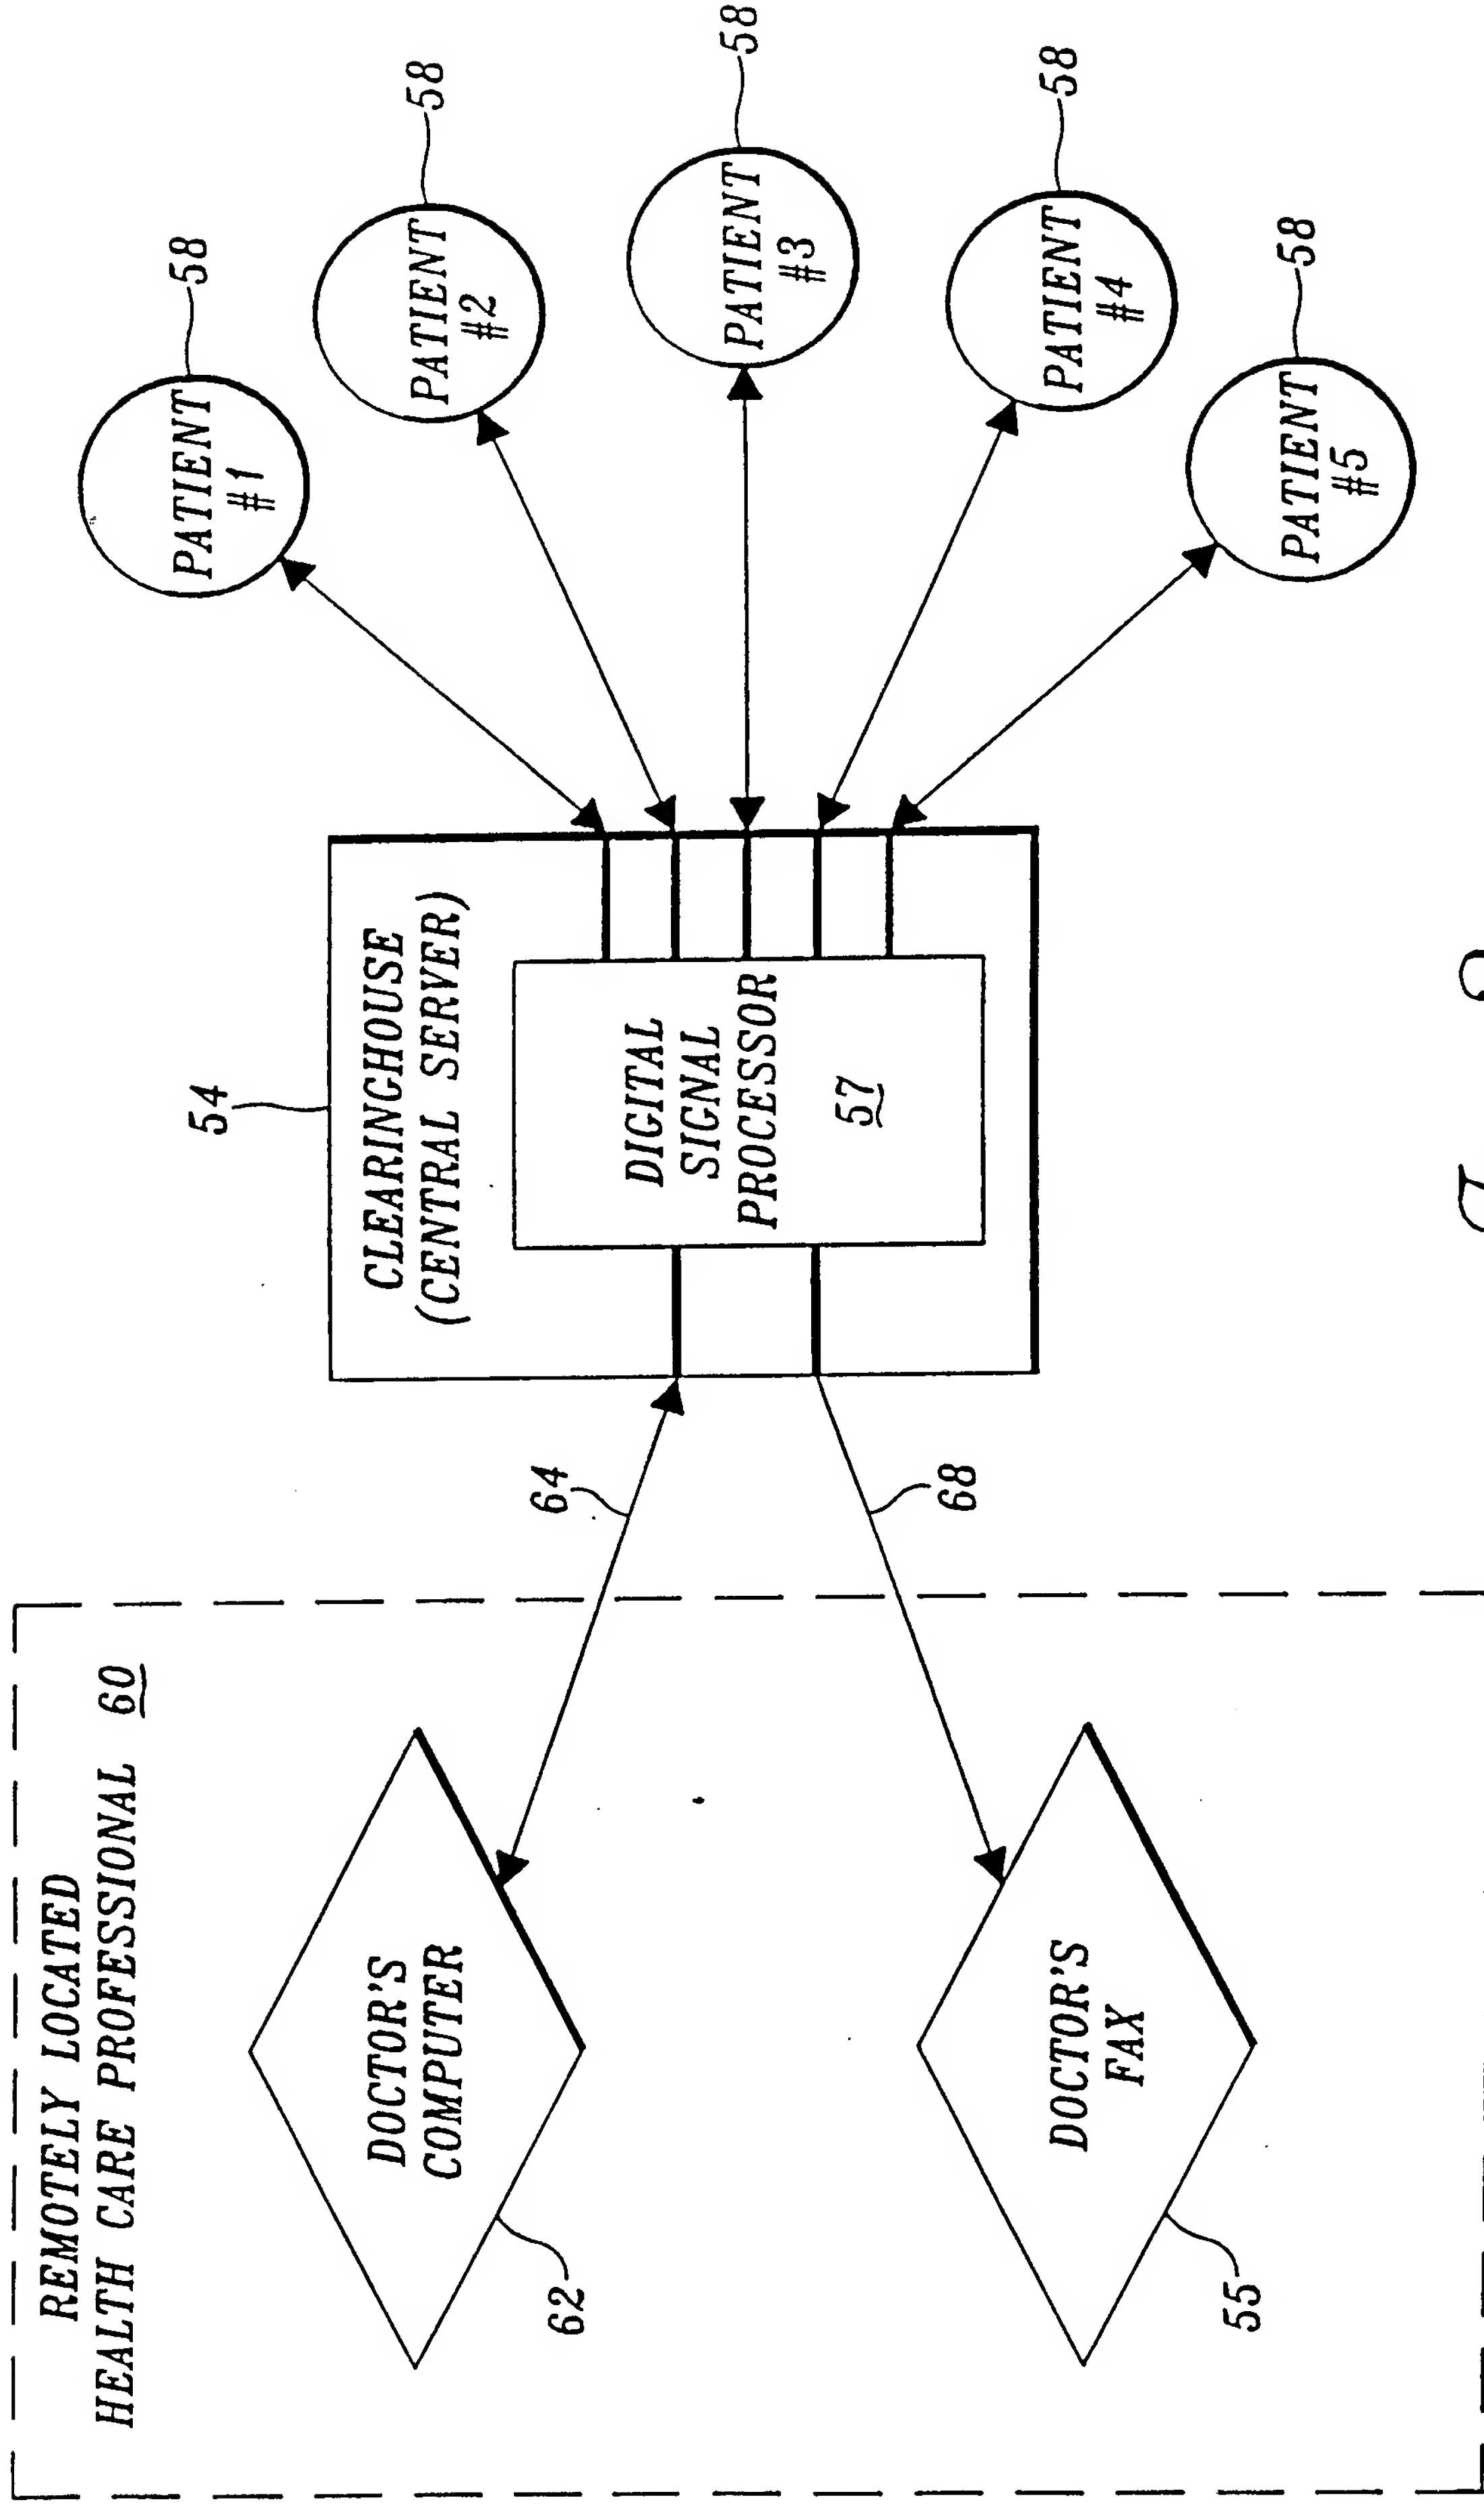


Fig. 2.

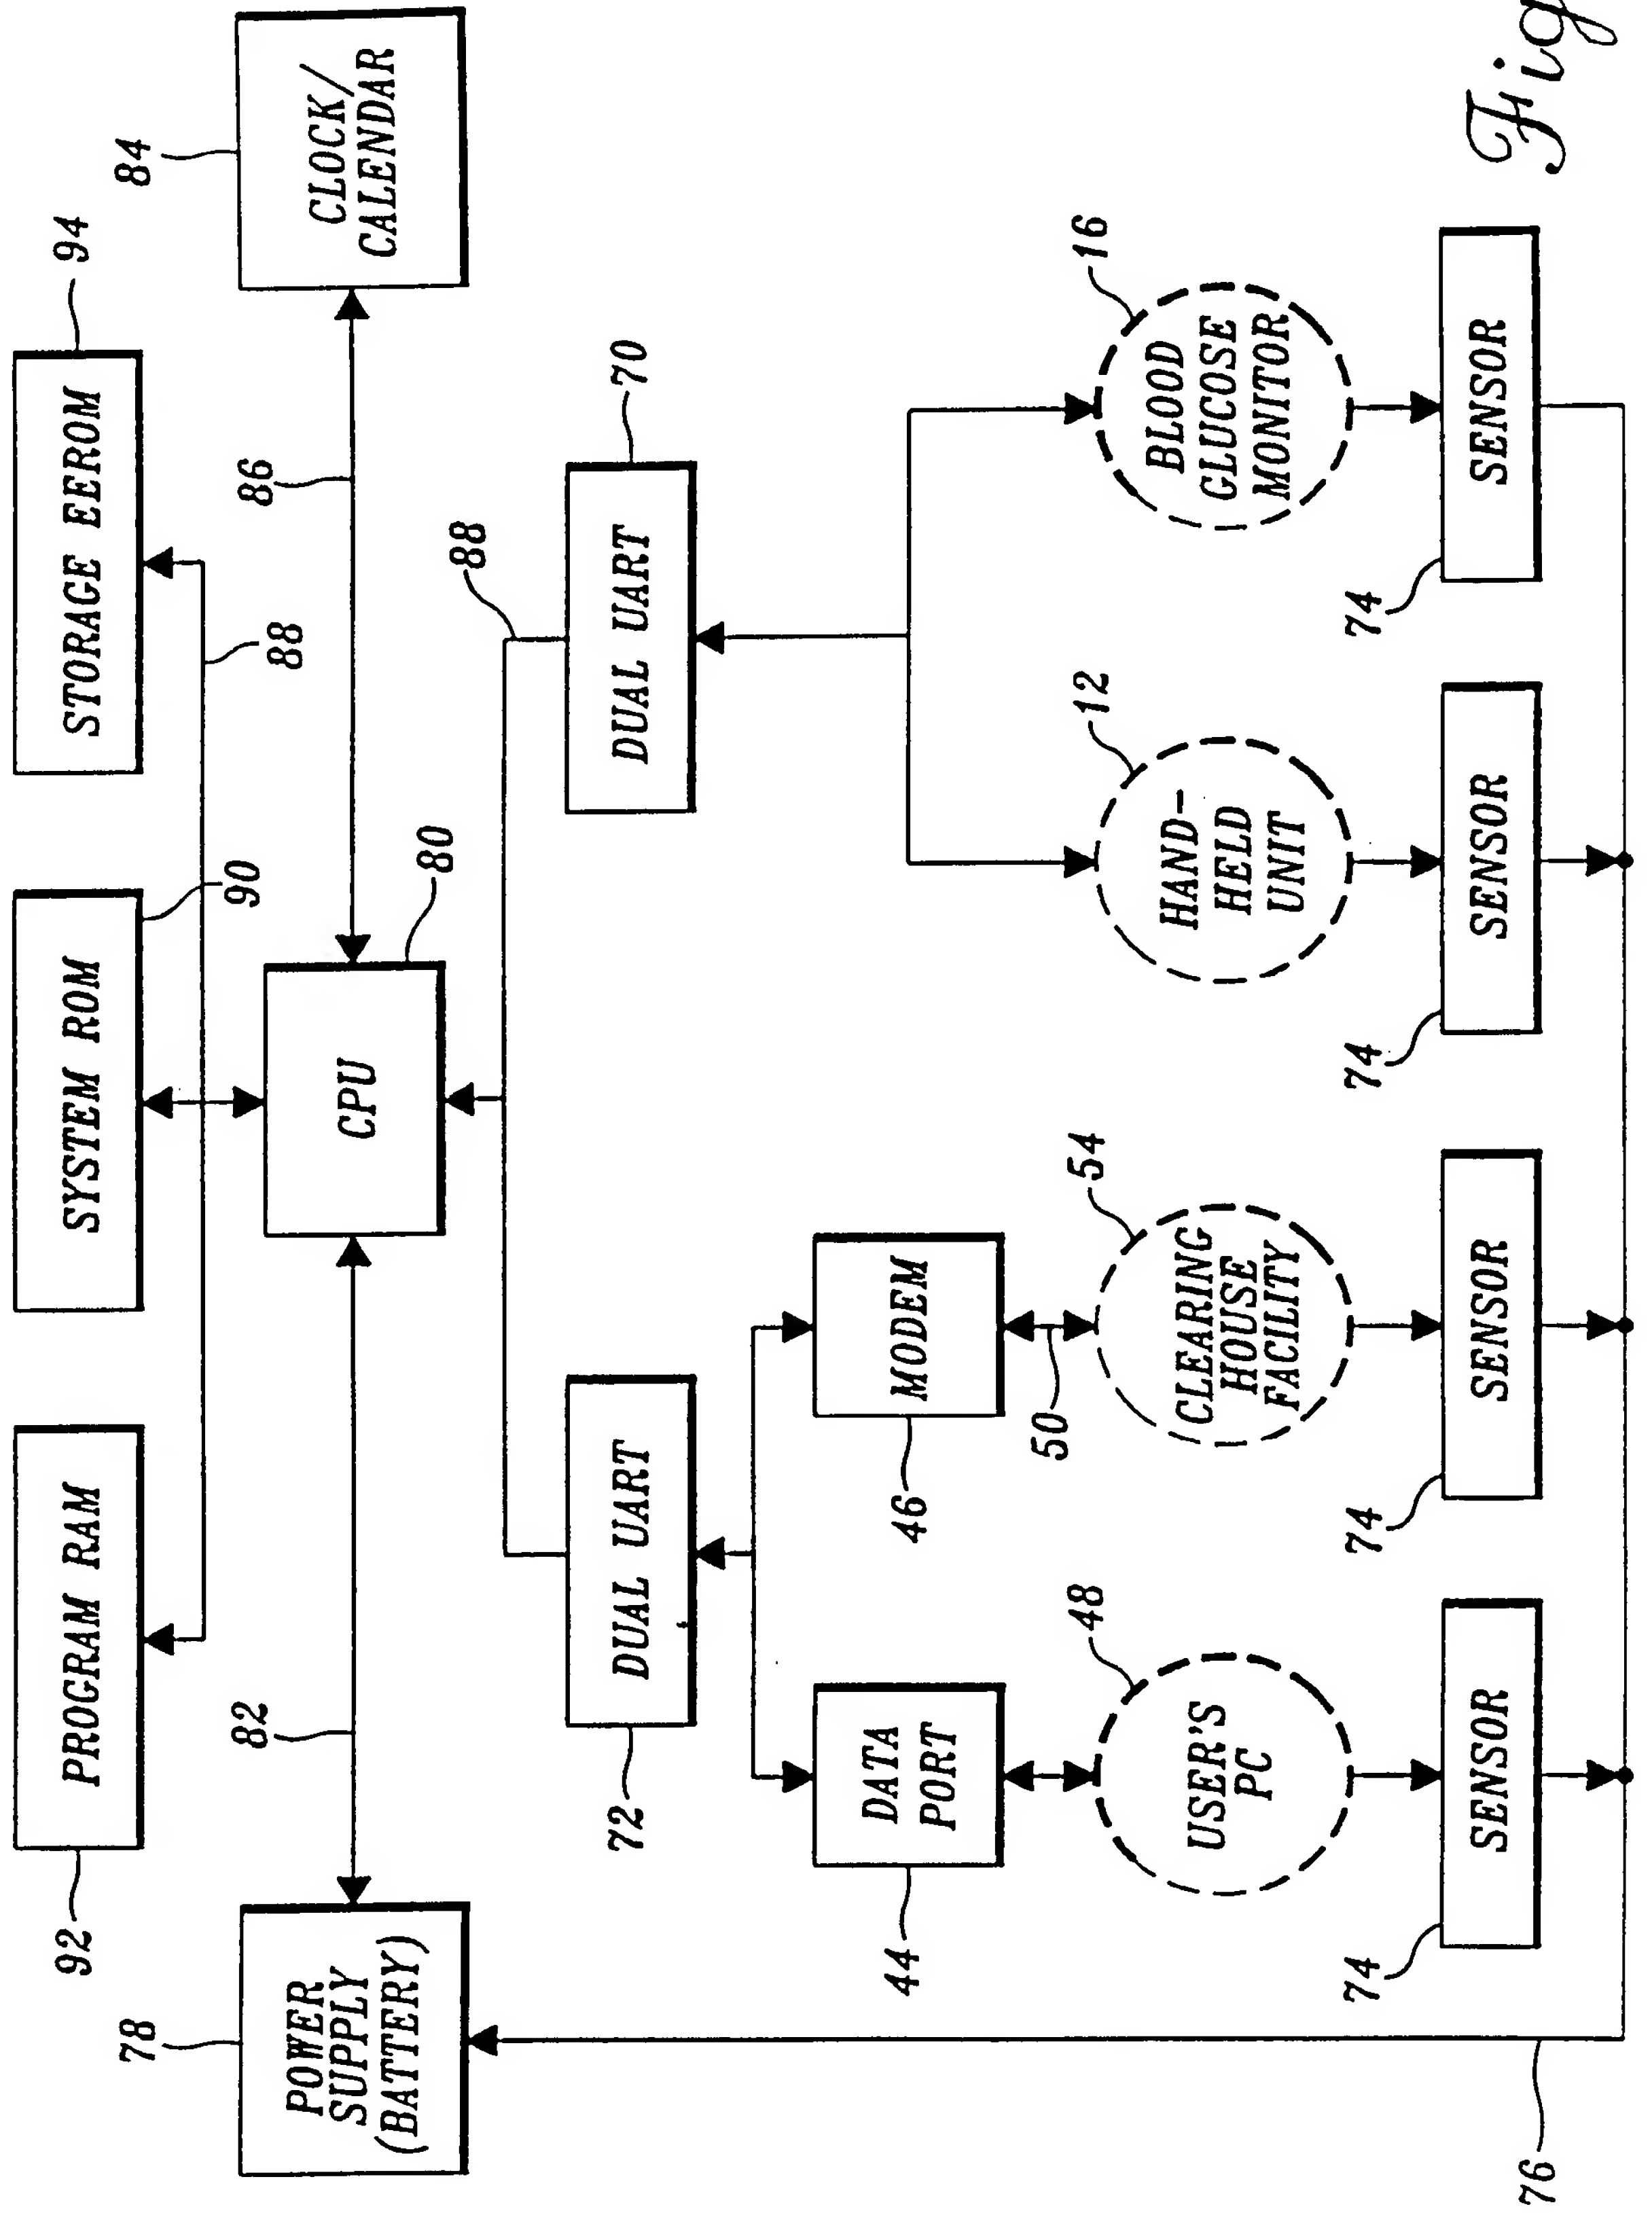


Fig. 3.

Fig.4.

Attention

Calibration was
not successful.

Please insert
the code strip
again.

Fig.5.

June 19 12:30 pm

Blood Glucose

109

mg /dl

remove test strip

Fig.6.

Mon Sept. 28 1992

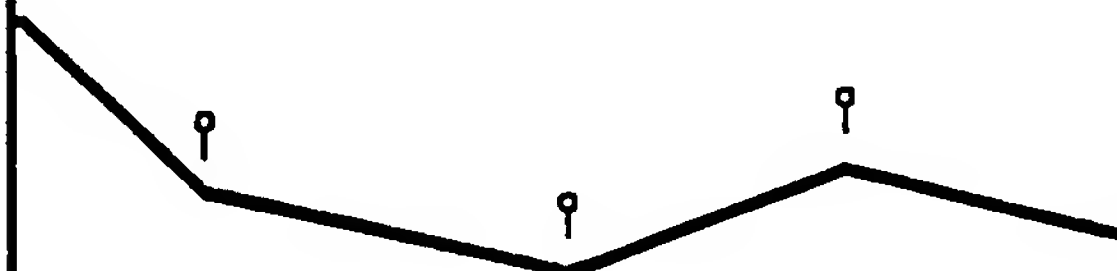


Fig.7.

Sept. 20-26 1992



Fig. 8.

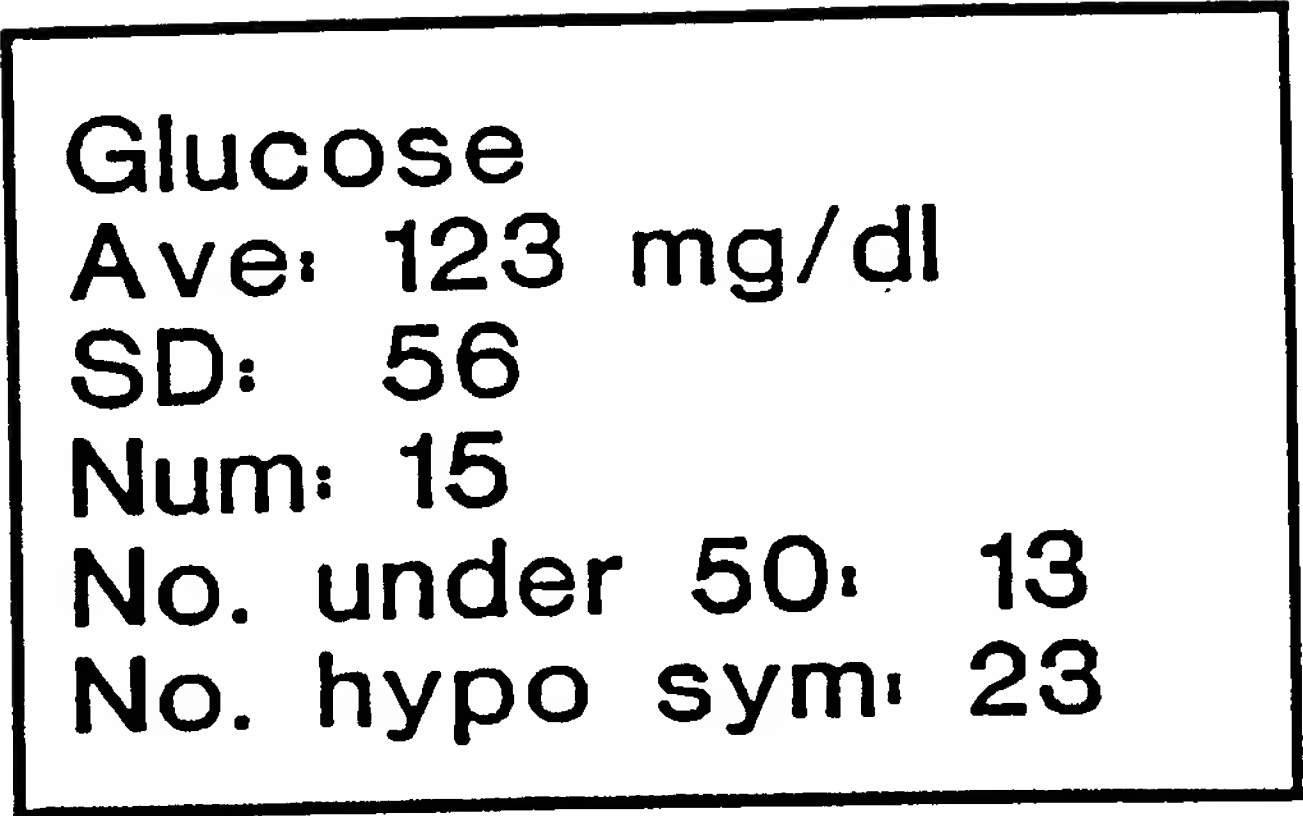


Fig. 9.

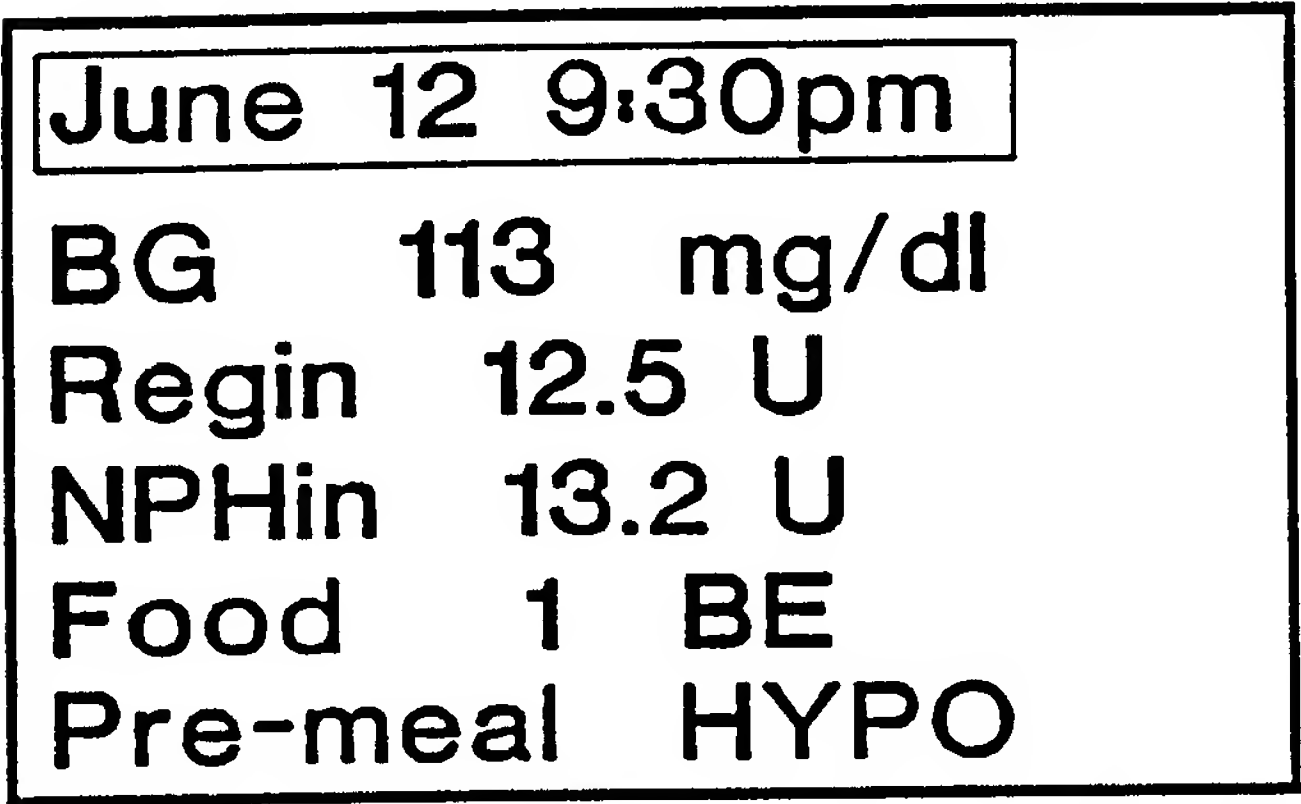


Fig. 10.

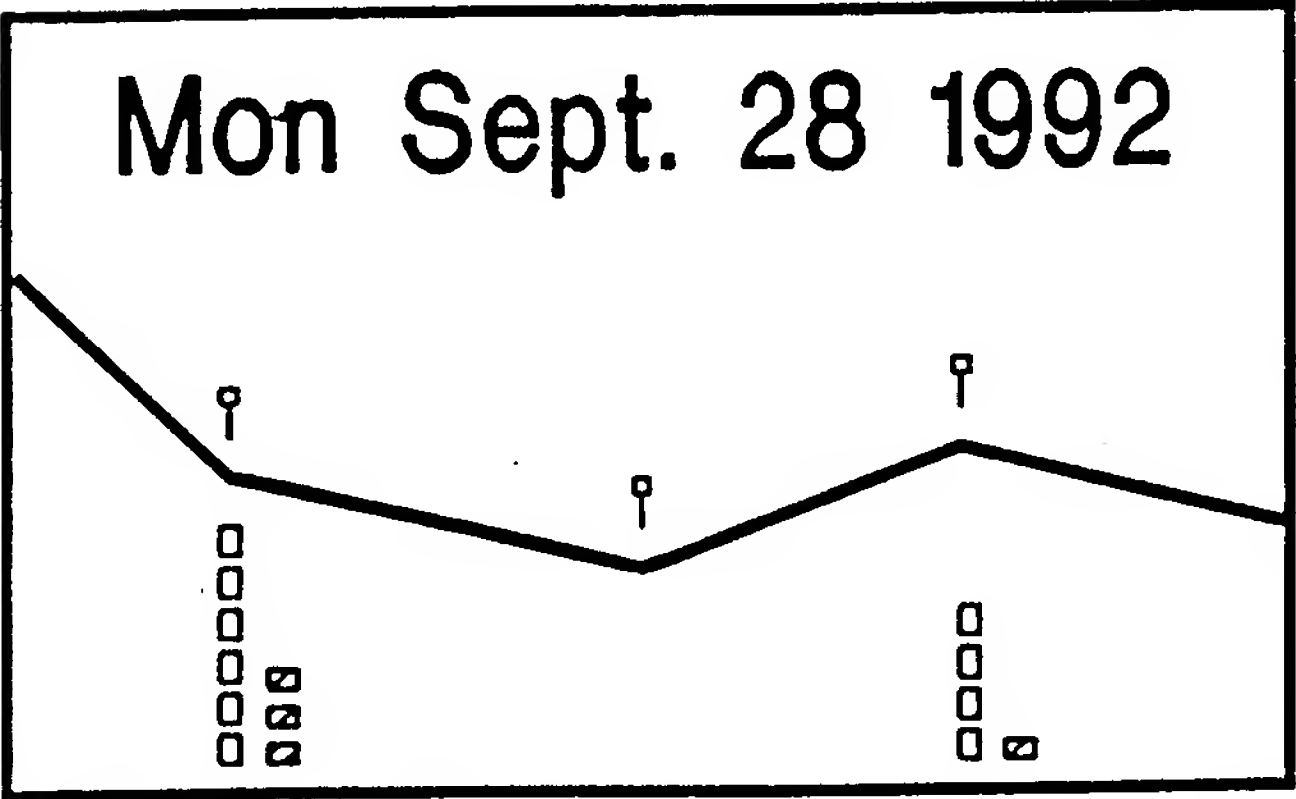


Fig. 11.

